
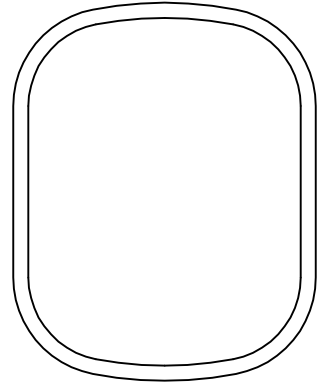



X120
2814
15141

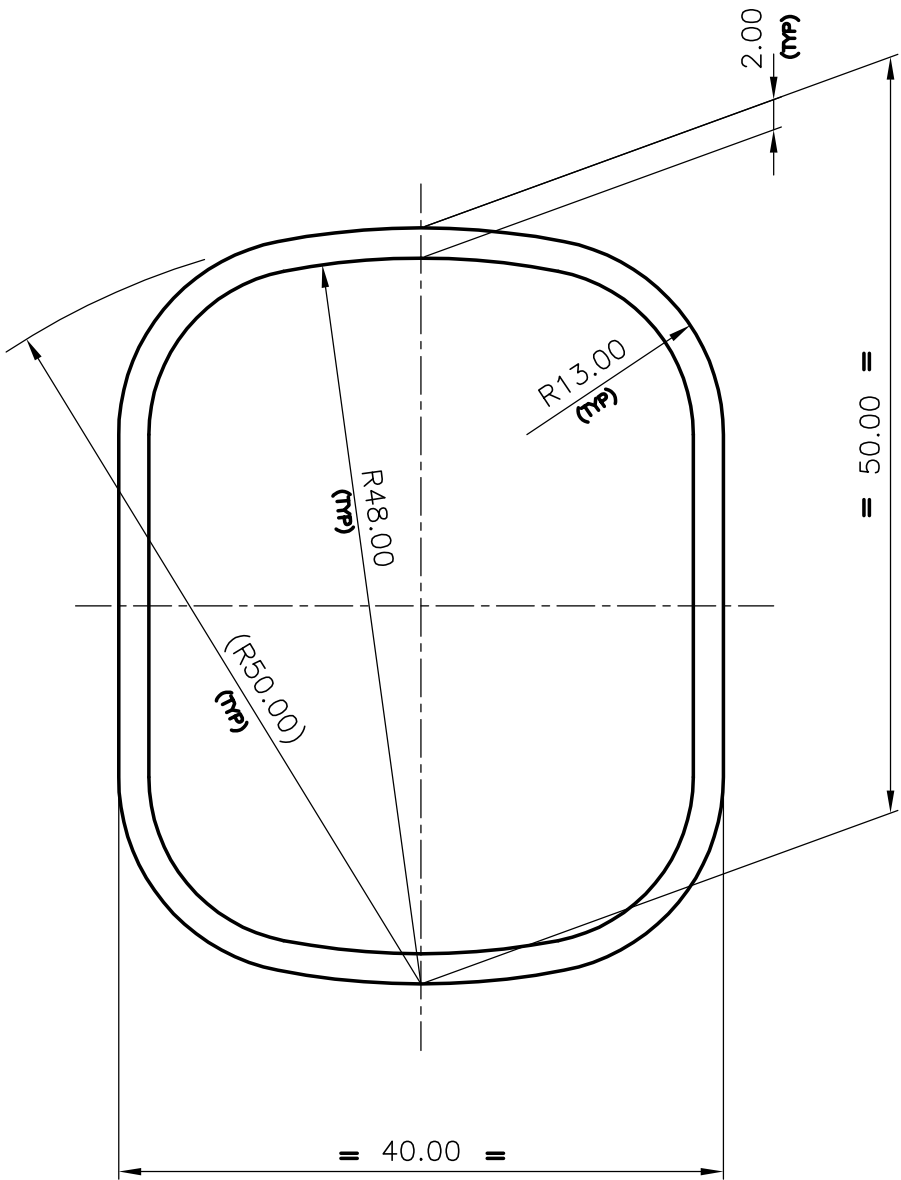

EXTRUDE ACTUAL PROFILE

GENERAL WALL THICKNESS 2.00 mm
 STRAIGHTNESS 1.70 mm/METRE OF LENGTH
 TWIST (1.5)° IN ONE METRE OR LESS OF LENGTH
 FLATNESS ±0.40 mm

 SYMBOL OF QUALITY AN ISO 9002 COMPANY	JINDAL ALUMINIUM LTD. BANGALORE-560073 (INDIA)	NAME	DATE
		DRAWN	P,KULKARNI 22-6-2000
1. ALL DIMENSIONS ARE IN mm. 2. ROUND OFF ALL SHARP CORNERS WITH 0.40 mm. 3. TOLERANCES WILL BE AS PER I.S. 6477-1983 UNLESS OTHERWISE SPECIFIED		CHECKED	
		APPROVED	
		SCALE	2:1
PARTY'S NAME	CONFIDENT DENTAL EQUIPMENT LTD, B'LORE.	WEIGHT kg/m	0.804
PARTY'S DRAWING No.	R & D HINGE 2	SECTION No.	15141
ALLOY & TEMPER	HE9 WP	DRAWING No.	
DESCRIPTION	COVER-LIGHT HINGE	15141	