


P-13797-1

X1773

28277

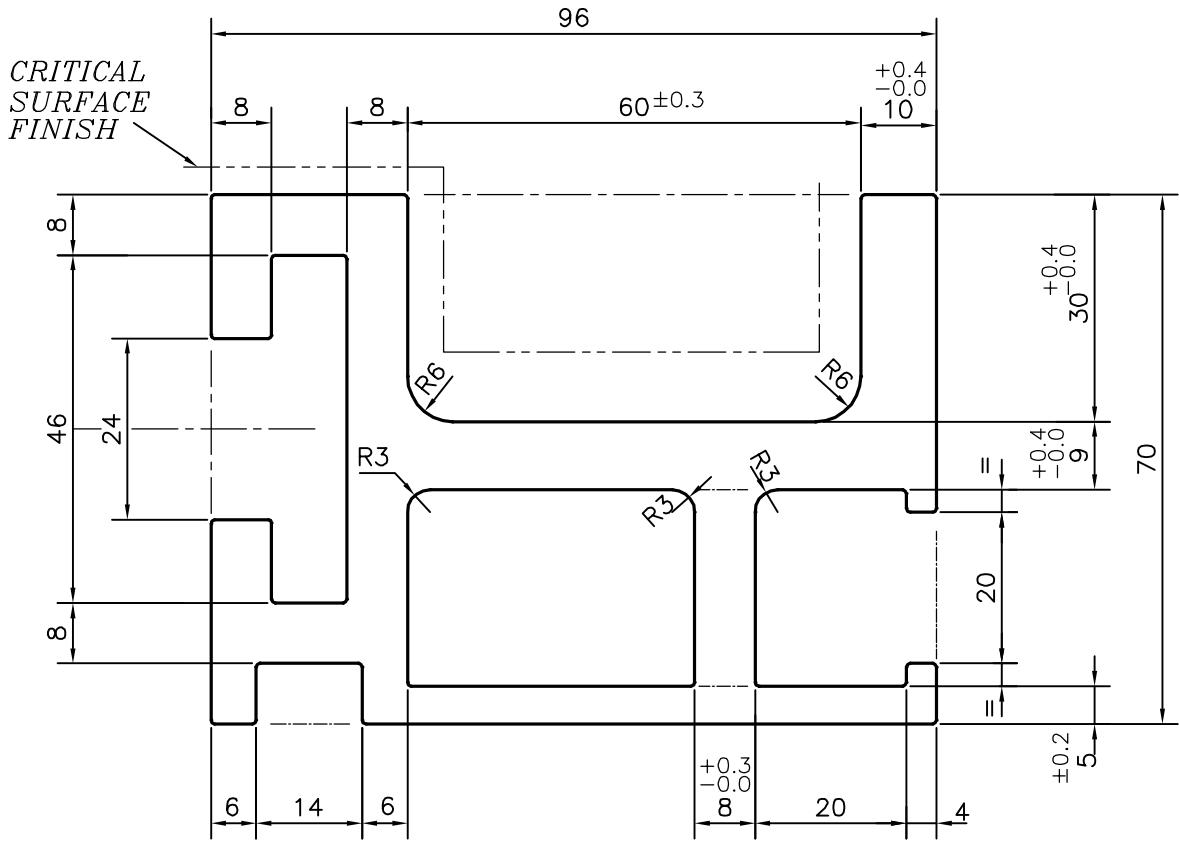

1. STRAIGHTNESS=0.7 mm/M
STRAIGHTNESS=3 mm/6 M
2. TWIST=0.7mm/M
TWIST=3 mm/6 M
3. ANGULARITY= ±0.5 mm.
4. FLATNESS =0.007xWIDTH



SYMBOL OF QUALITY
AN ISO 9001 COMPANY

JINDAL ALUMINIUM LTD.
BANGALORE-560073 (INDIA)

	NAME	DATE
DRAWN	PARVESH	04-08-2014
CHECKED		
APPROVED	S.S.GARG	11-08-2014
SCALE		1:1
AREA mm ²		2589.016
PERIMETER mm.		536.283
WEIGHT kg/m		6.99
DRAWING No.	SECTION No.	
P-13797-1	-	
X1773	X1773	
28277	28277	

1. ALL DIMENSIONS ARE IN mm.
2. ROUND OFF ALL SHARP CORNERS WITH 0.50 mm.
3. TOLERANCES WILL BE AS PER BS:EN-12020-2 , UNLESS OTHERWISE SPECIFIED

PARTY'S NAME	PROGNOSYS MEDICAL SYSTEMS PVT. LTD., BANGALORE
PARTY'S DRAWING No.	AS PER DRAWING
ALLOY & TEMPER	6005 T6
DESCRIPTION	INDUSTRIAL SECTION-MEDICAL